



# NVAMD Examinations Using Different OCT Systems

## NVAMD Pathology Identified

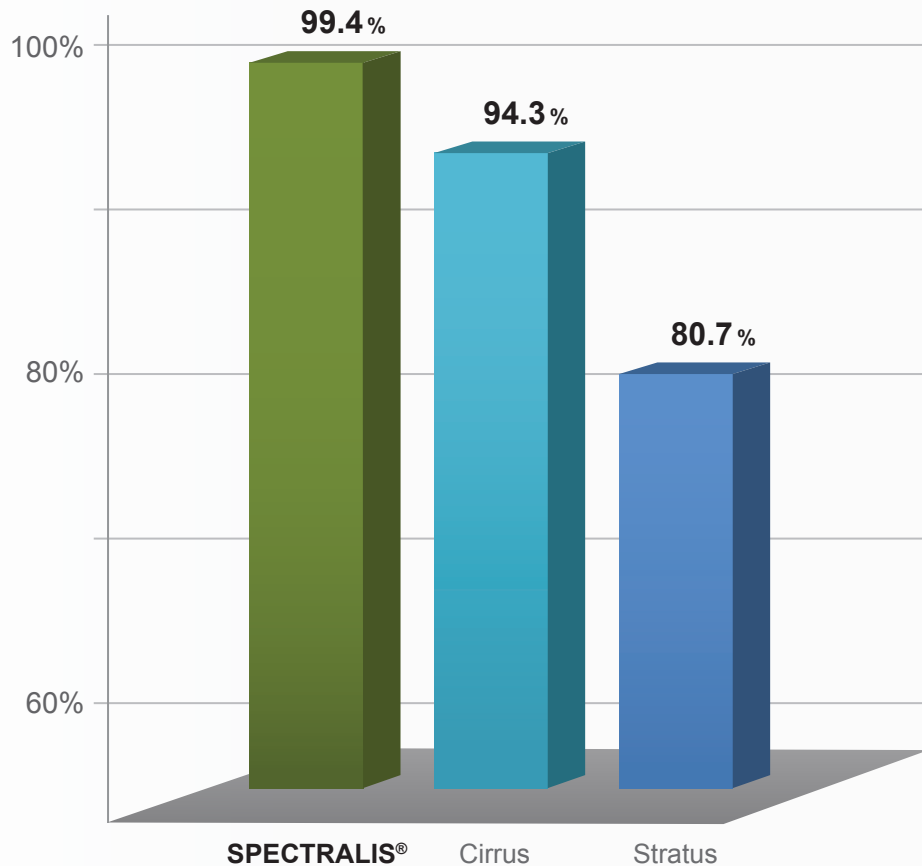

## Intra Retinal Fluid Missed

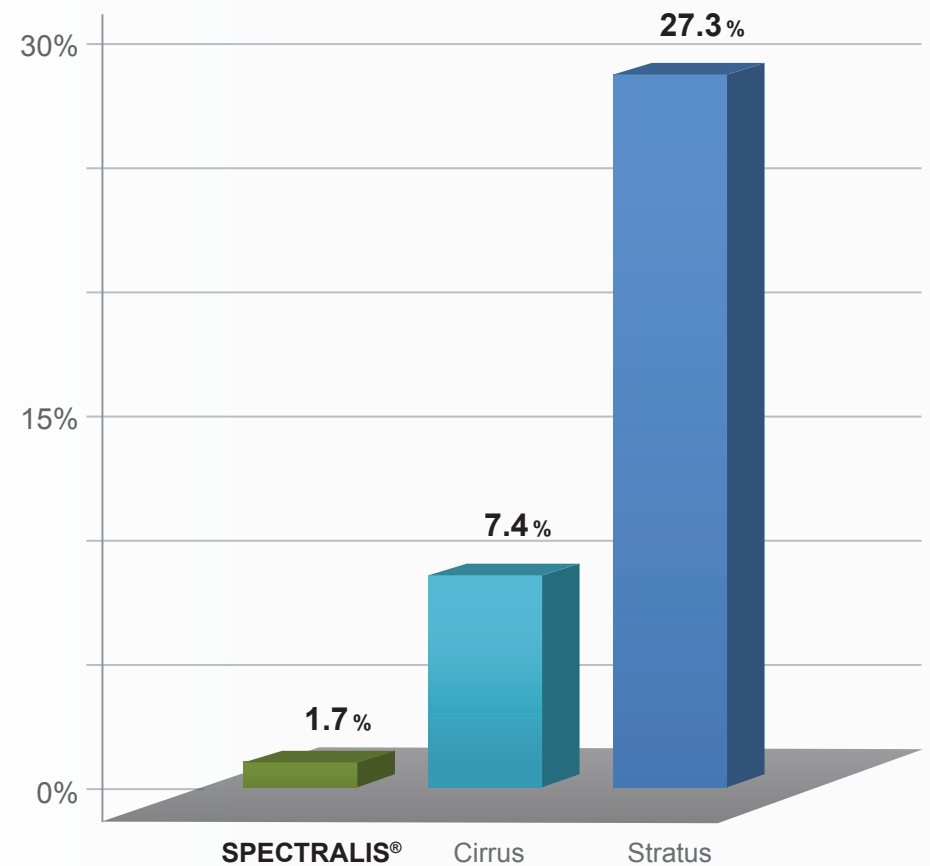

*D.M. Brown, A. Mariani, E. Kegley, J.C. Major.*

### Optical Coherence Tomography in the Management of Neovascular Age-Related Macular Degeneration: A Comparison of Spectral-Domain and Time-Domain Retinal Imaging Systems

Presented at the 2011 ARVO/ISIE Imaging Conference, program number 52: [www.arvo.org/isie](http://www.arvo.org/isie). Data from the SAVE trial, a Genentech sponsored study involving multiple examinations of 50 AMD patients to assess relative sensitivity of commonly available OCT machines in a population with a high prevalence of retinal pathology, presented at ARVO and ASRS (2011).

SPECTRALIS is a registered trademark of Heidelberg Engineering Inc. or Heidelberg Engineering GmbH.  
© 2011, Heidelberg Engineering, Inc. All rights reserved. 2476  
All trademarks are the property of their respective owner.

